


## Orientation

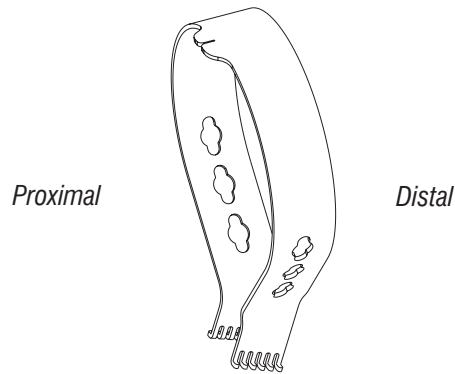

CANICA®

## PalmSpring®

### Instructions for Use

## Sterilization and Cleaning

**NOTE:** All reusable components are supplied in a non-sterile condition.  
The CHESS® Elastomer is sold separately and supplied sterile, for single use only.


### Sterilization:

The following sterilization procedure should be followed prior to use:

Process: Prevacuum Steam Autoclave  
Temperature: 270°F (132°C)  
Time: 4 minutes

### Cleaning:

After use, all reusable components should be cleaned manually with soap and water or by ultrasonic methods.

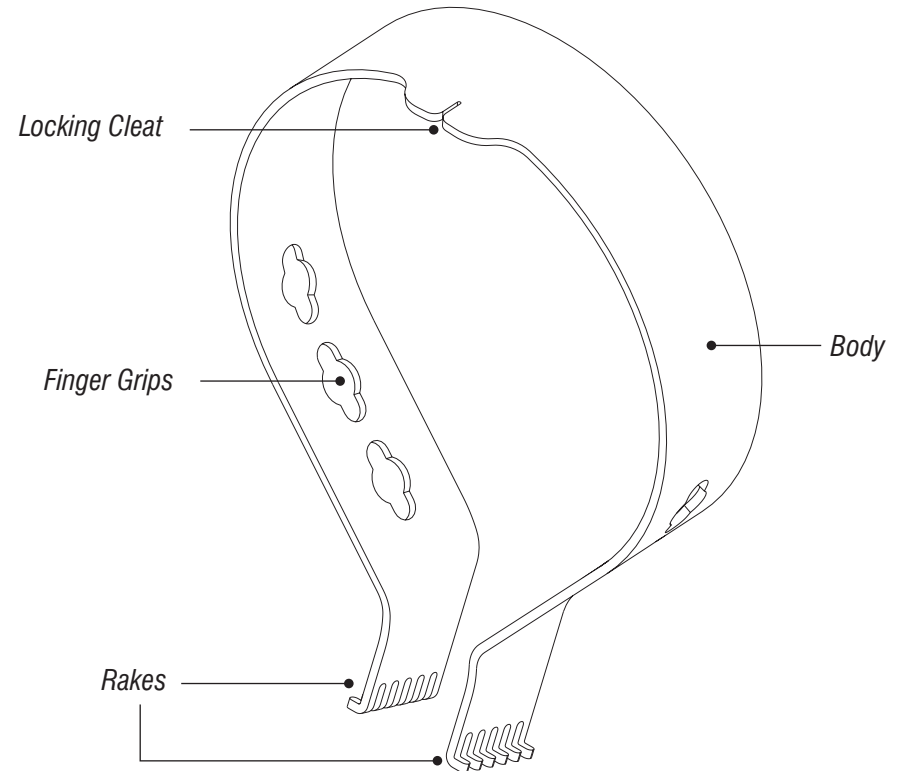

## Order Information

Description	Part Number
PalmSpring®	CCPS1



CEpartner4U  
3951DB; 13. NL.  
Tel: +31(0)6.516.536.26

CANICA®

Canica Design Inc.  
Head Office  
36 Mill Street, Almonte, ON Canada K0A 1A0  
U.S. Distribution Center  
814 Proctor Ave, Ogdensburg, NY USA 13669-2205


Phone: 1-613-256-0350  
Fax: 1-613-256-0360  
Email: sales@canica.com  
Toll Free: 1-800-705-8312  
Web: www.canica.com

### INDICATIONS FOR USE:

PalmSpring® is a self-retaining deep tissue retractor for small palmer incisions, which creates a 2 cm x 2 cm surgical aperture from a 2 cm incision.

## Instructions for Use




**Adjusting Tension:** Adjust the retractive force by bending the rakes inward or outward.

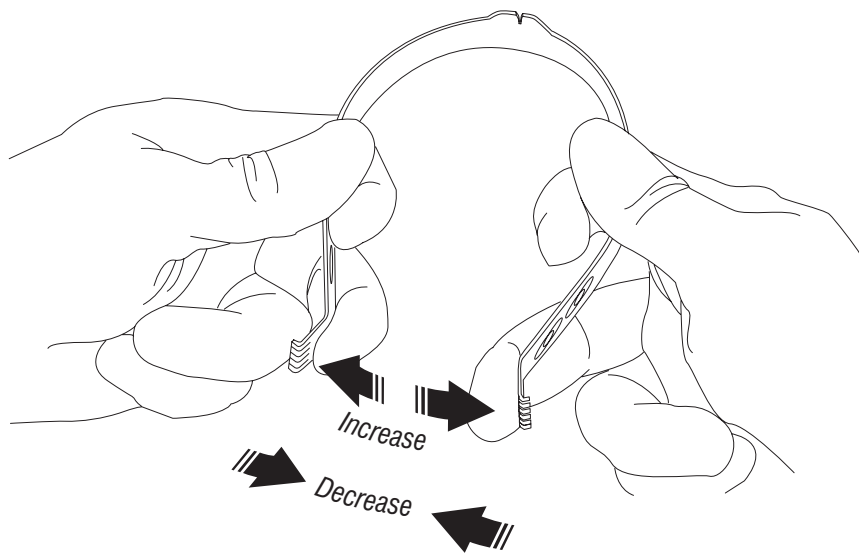

The PalmSpring is a malleable, spring-type retractor. Force is adjusted by bending the rakes inward or outward.





### Step 1 - Installing the PalmSpring

- Compress the body until rakes touch. (Figure A)
- Insert PalmSpring into incision. (Figure B)
- Release grip. (Figure C)



### Step 2 - Adding a Proximal Fat Pad Lifter

- Fasten CHES<sup>®</sup> elastomer to retractor. (Figure D)
- Position retractor. (Figure E)
- Secure elastomer to the cleat. (Figure F)



## Procedure Configuration

### Carpal Tunnel Release

The PalmSpring can be used alone or in combination with the Canica CHES<sup>®</sup> Surgery System.

